


AEG 31 GWU



Schalter	2	3	4	5	6	7	8	9	10	11	12	13	15
TA													
Lang													
Mittel													
Kurz													
UKW													

Messinstrument: 333Ω/V

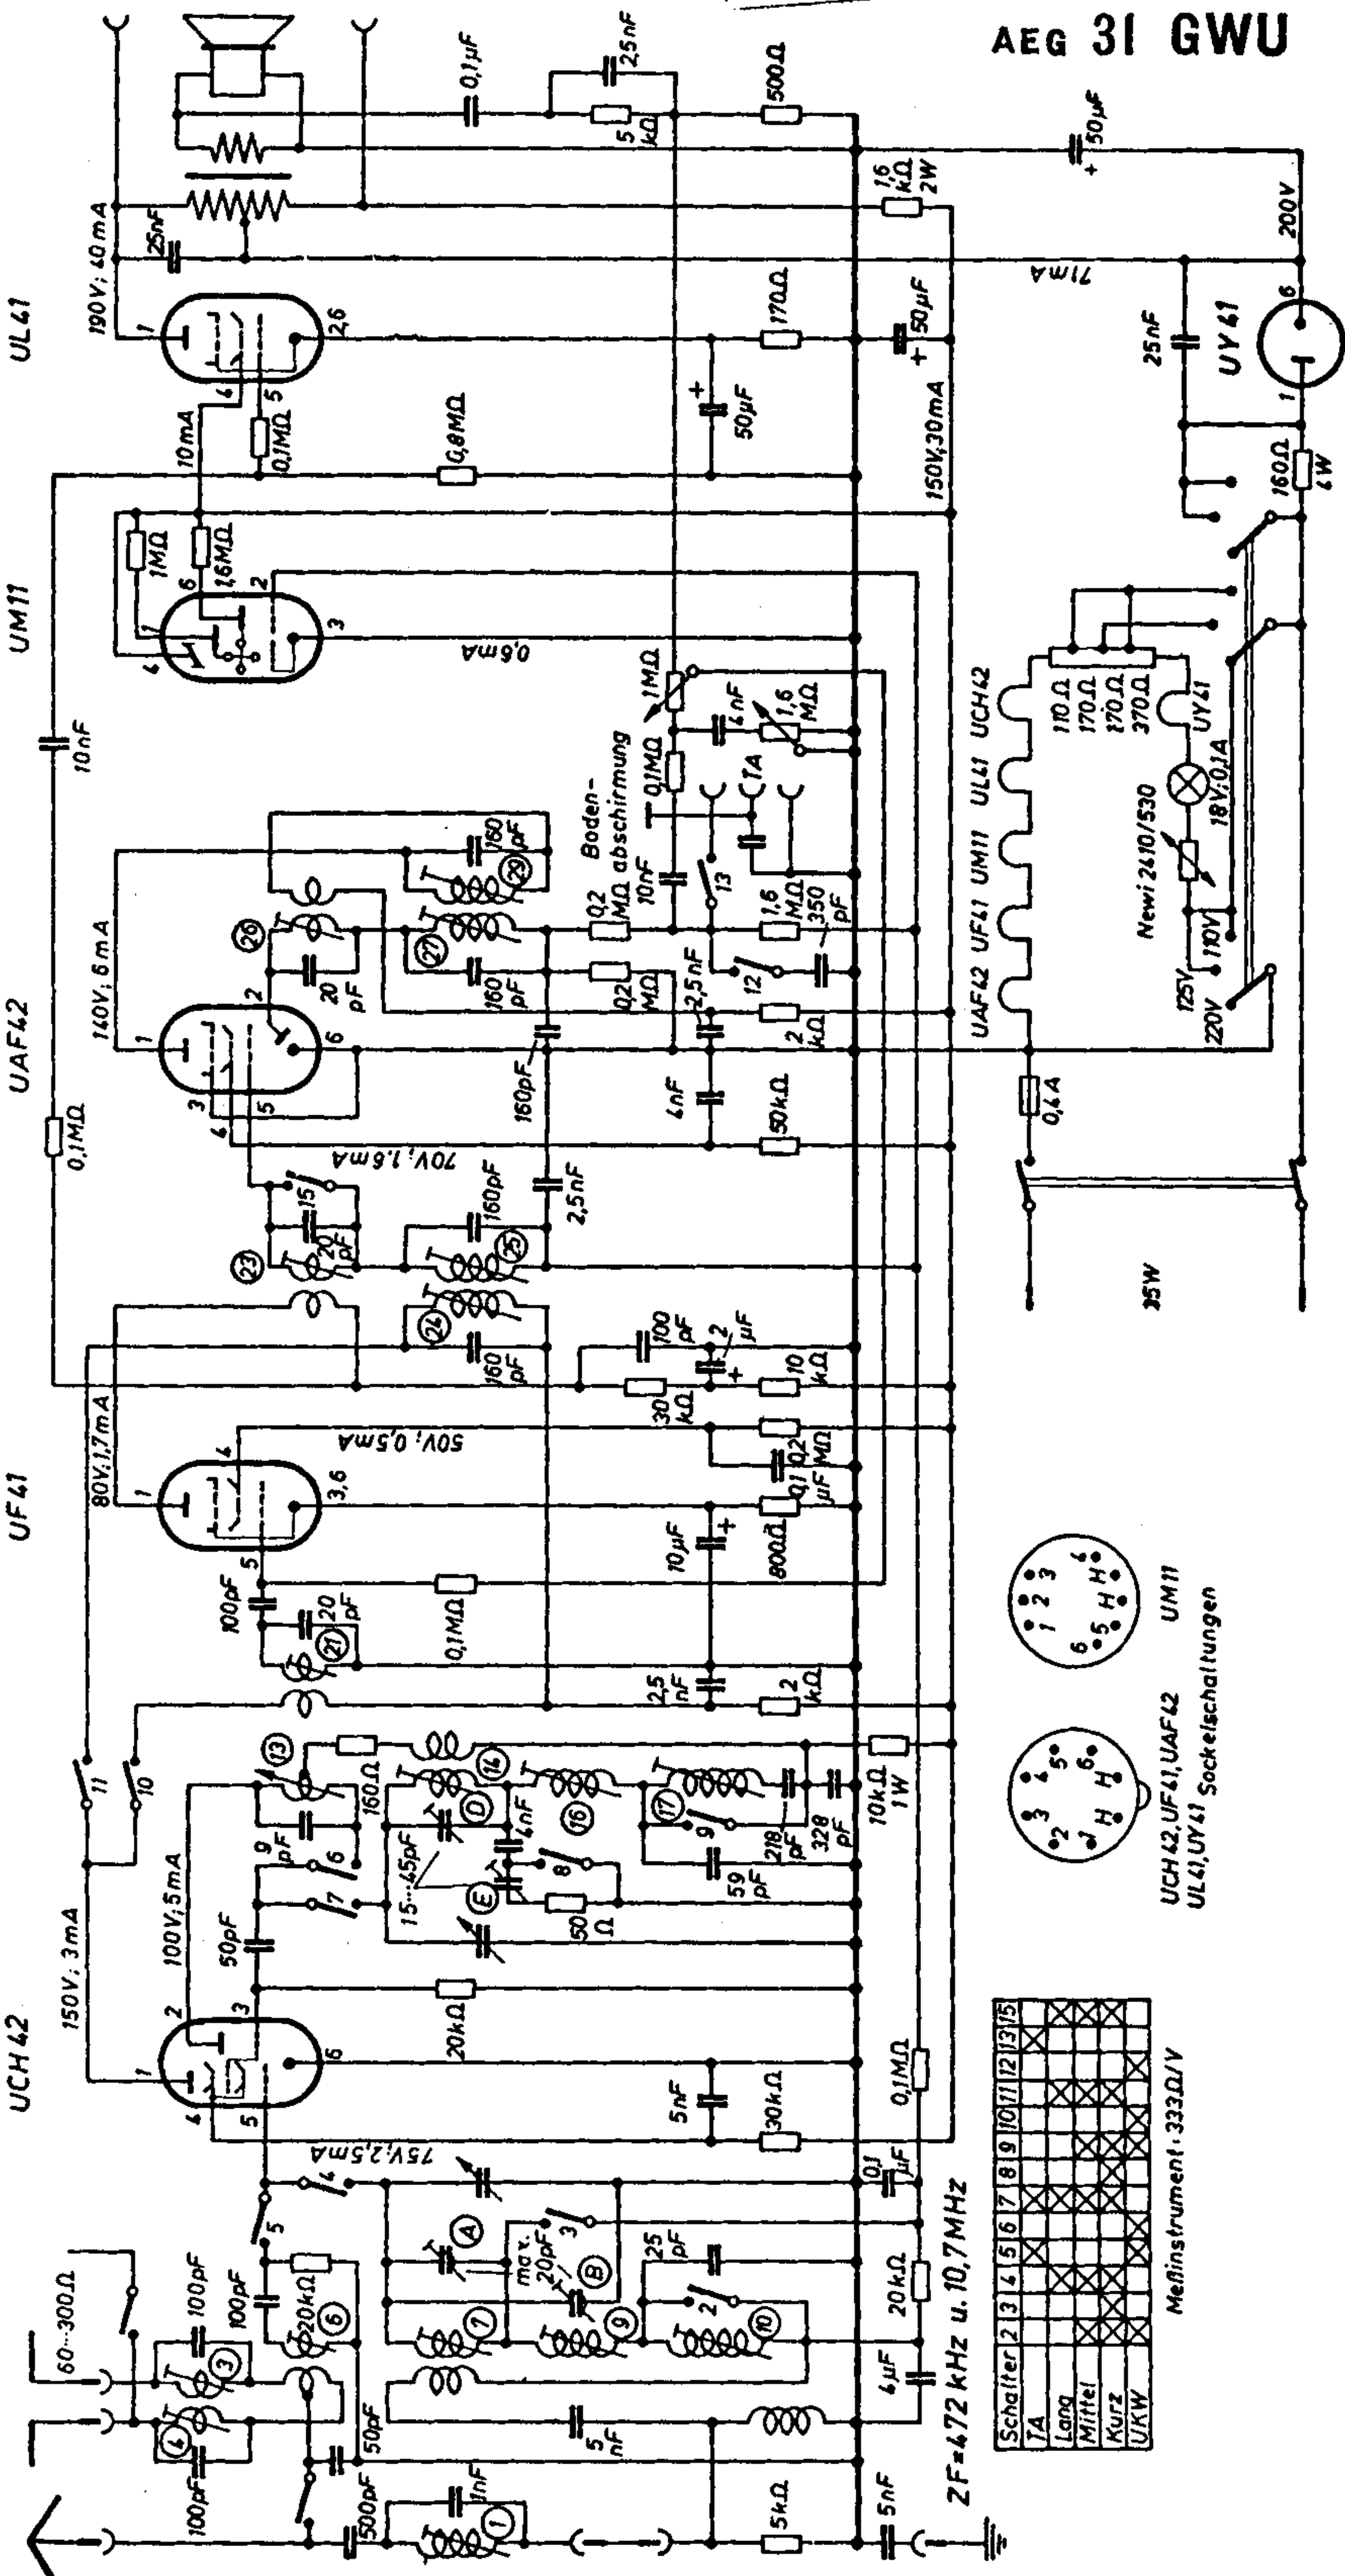

UCH42, UF41, UAF42  
UL41, UY41 Sockelschaltungen

25W

71mA

25nF

160Ω

2W

18V/0,1A

125V

220V

0,4A

25W

170Ω

170Ω

370Ω

UY41

160Ω

2W

1

6

200V

50μF

150V, 30mA

50μF

170Ω

500Ω

5kΩ

25nF

5kΩ

5nF

0,1μF

20kΩ

4μF

5nF

0,1MΩ

10kΩ

1W

328 pF

218 pF

59 pF

2 kΩ

2,5 nF

10 μF

800Ω

0,1 μF

0,1 MΩ

100 pF

30 kΩ

700 pF

2 μF

10 kΩ

350 pF

1,6 MΩ

2 nF

1,6 MΩ

1 MΩ

0,1 MΩ

10 nF

0,2 MΩ

10 nF

160 pF

2,5 nF

160 pF

15 pF

20 pF

160 pF

70V, 1,6mA

0,2 MΩ

10 nF

0,2 MΩ

10 nF

1 MΩ

0,1 MΩ

1 MΩ

1 MΩ

15 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ

10 MΩ

1 MΩ